Elisys Uno

| Unpacking Instruction

CE

Cat.No. 17350/4

Human

Revision List of the Manual		
No.	Rev. / DATE	REVISION DESCRIPTION
1	01/2006-08	First edition
2	02/2008-05	Adaptation to new Corporate Design

Contents

1	UNPACKING INSTRUCTIONS ELISYS UNO	3
2	Instrument Set-Up	6

1 UNPACKING INSTRUCTIONS ELISYS UNO

NOTE:	SAVE ALL PACKING MATERIAL FOR FUTURE USE

1) **To open the crate:** Remove security locks from each latch (2) located on the right front corner of the crate. Use caution when opening the latches. **SEE ILLUSTRATION ATTACHED TO SHIPPING CRATE.**

2) Pull the instrument package assembly out by the bottom cardboard skid.

CAUTION:	To prevent the backside of the instrument from dropping off the crate, support the backside of the instrument before pulling the instrument all the way out of the crate.

3) Remove the accessory box. Remove the stretch wrap holding the end caps in place and remove the foam end caps.

4) Lift the ELISYS UNO off the cardboard skid and place it on a stable working surface for further unpacking.

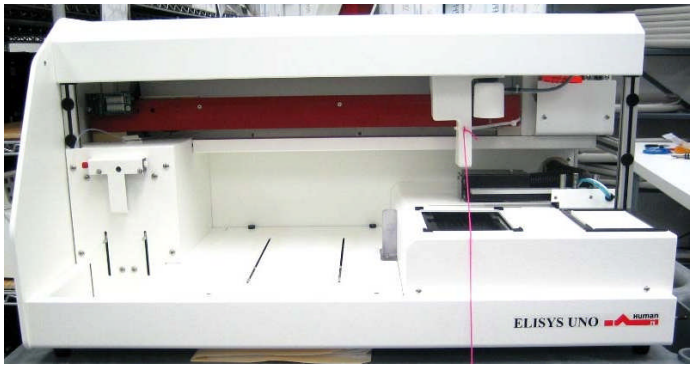

5) Remove the two (2) screws that hold the interior plate cover and slide the cover out through the front of the instrument.

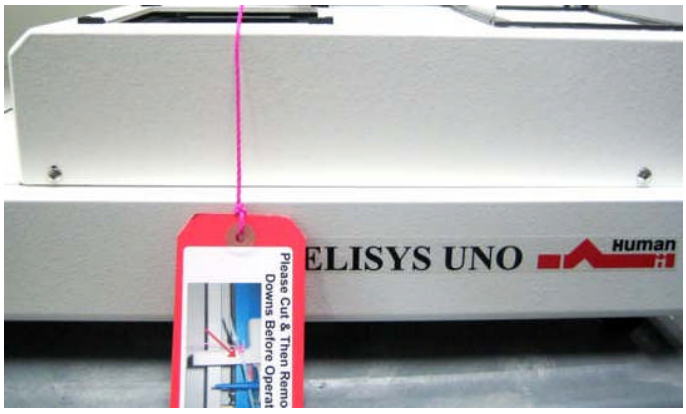

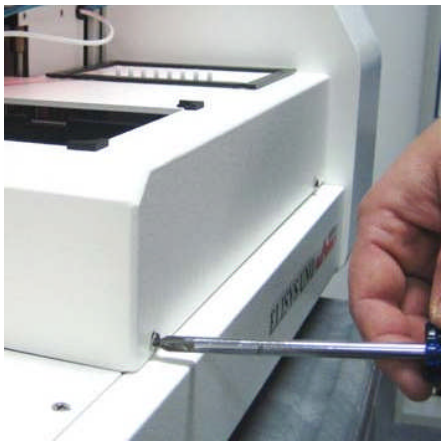

6) Cut the tie wraps that secure the packing splints at the front right and left rear of the mover shaking platform and remove the tie wraps and packing splints.

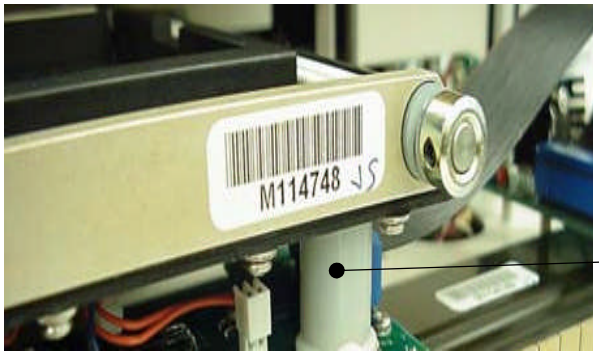

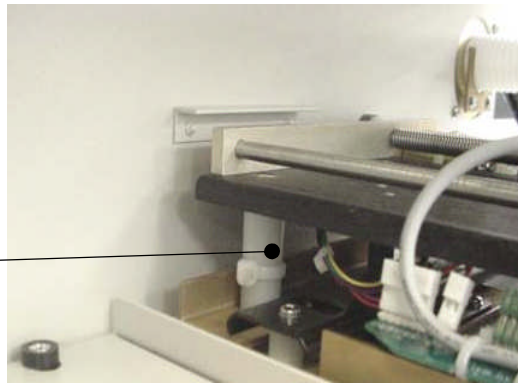

7) Remove the shipping bracket from the front of the plate mover undercarriage.

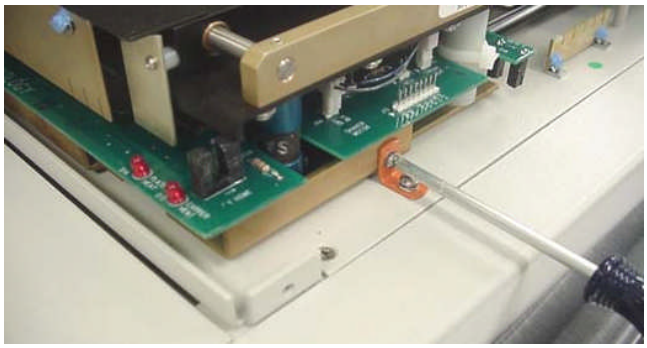

8) Cut the tie wraps that secure the Probe Z for shipment and remove the tie wraps and tag

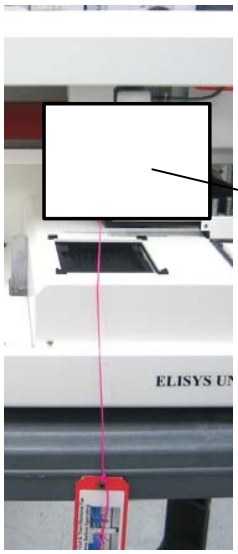

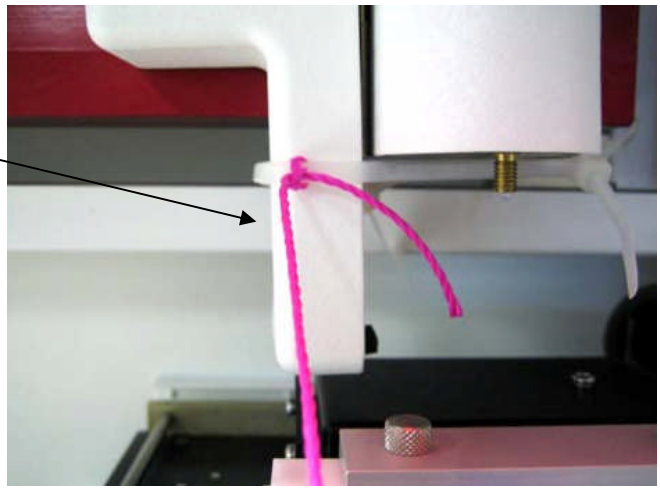

9) Remove the green valve support blocks from the Rinse and Wash Dispense valves by pulling them toward the front of the unit.

Warning:	**If the valve support blocks are not removed, the photometer will be flooded with fluids when a wash or rinse command is issued.**

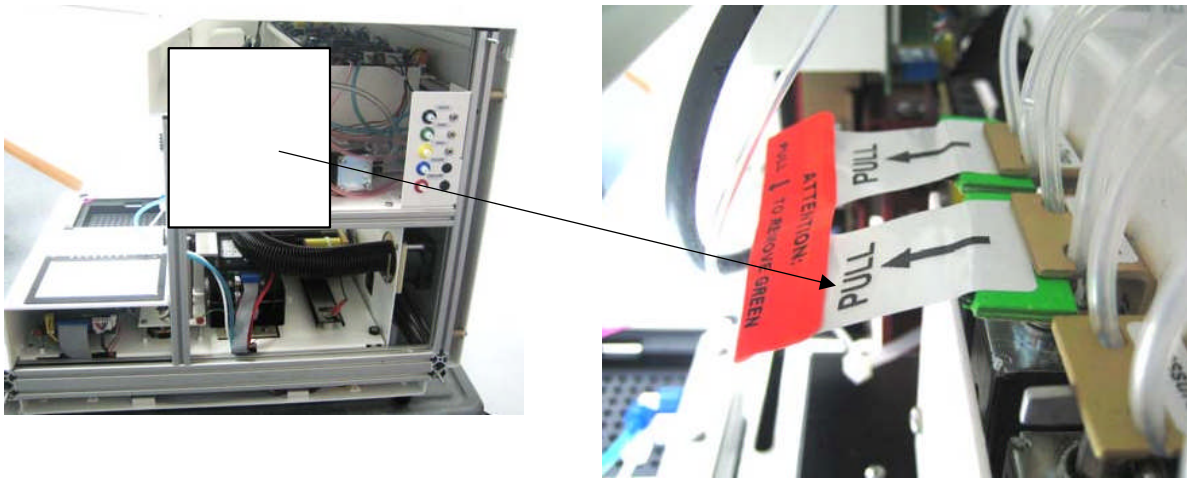

10) Remove (3) Rosette Nuts

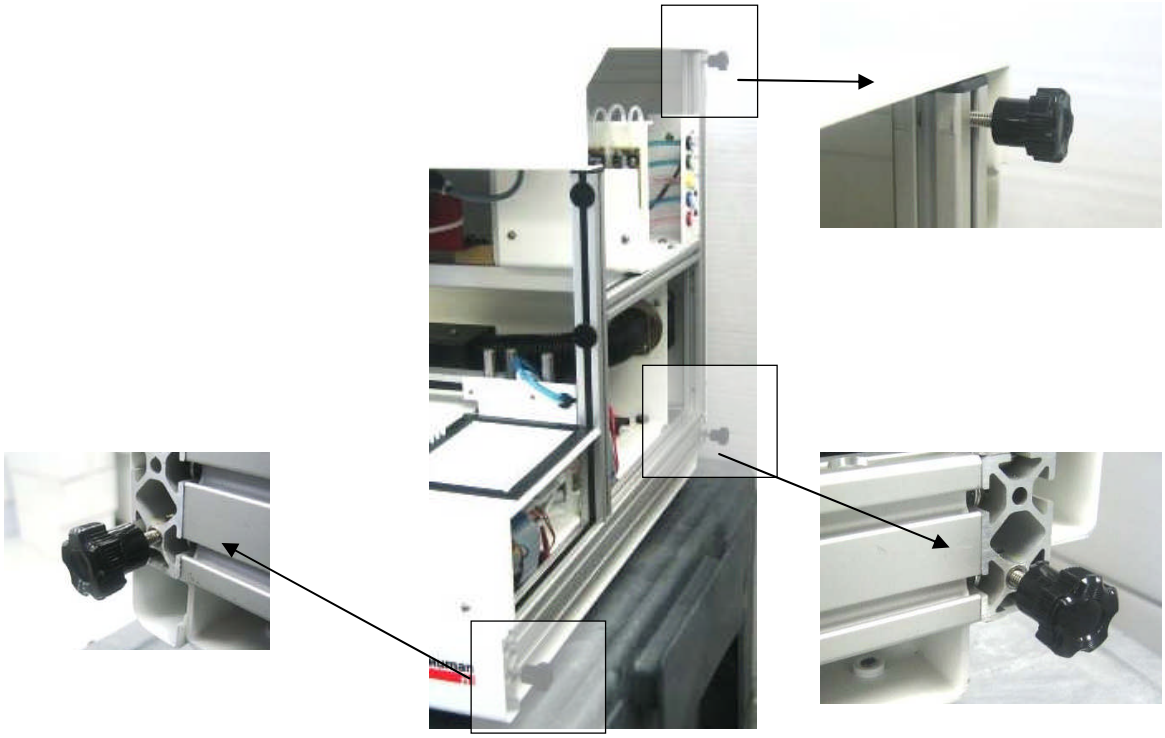

2 Instrument Set-Up

11) Pull Probe tip and Blue Probe Tip Support from Spare Parts Kit

a. Remove probe tip from plastic tube

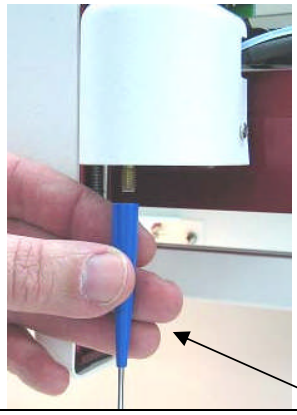

b. Insert Probe tip into blue probe support

12) Twist probe tip onto the probe **FINGER TIGHT**

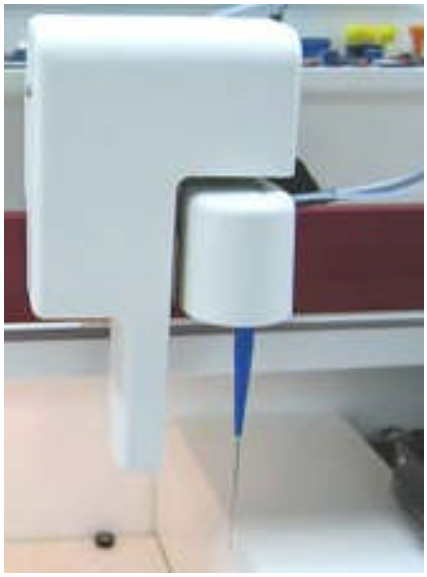

13) Remove 8 Way Wash head from packaging

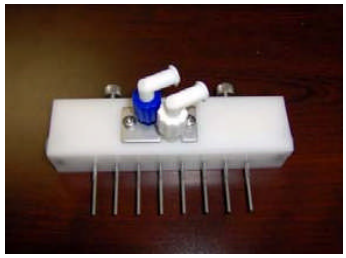

14) Install into probe arm once unit is powered and arm has raised completely

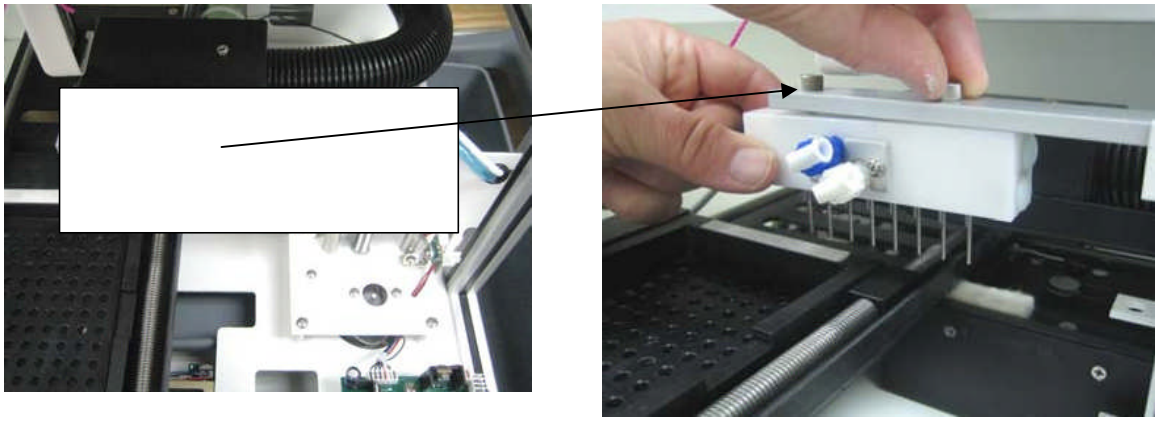

15) Mount side bottle enclosure to the right side of unit

Step 1: Line up 3 unit pins with 3 side panel holes

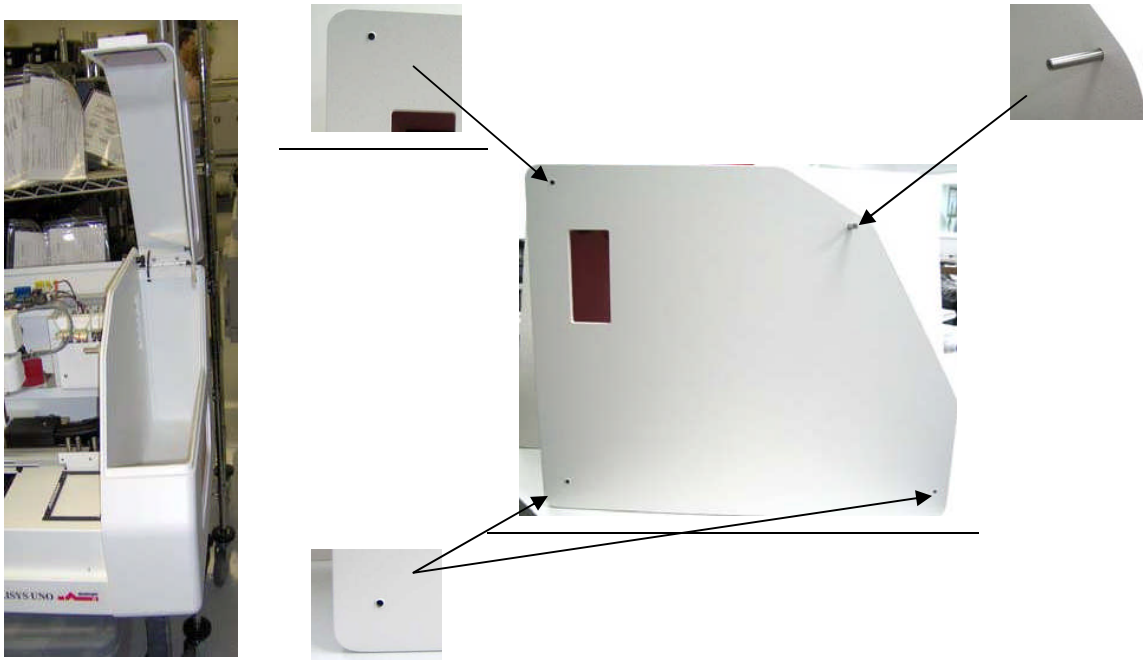

16) Install front cover to unit

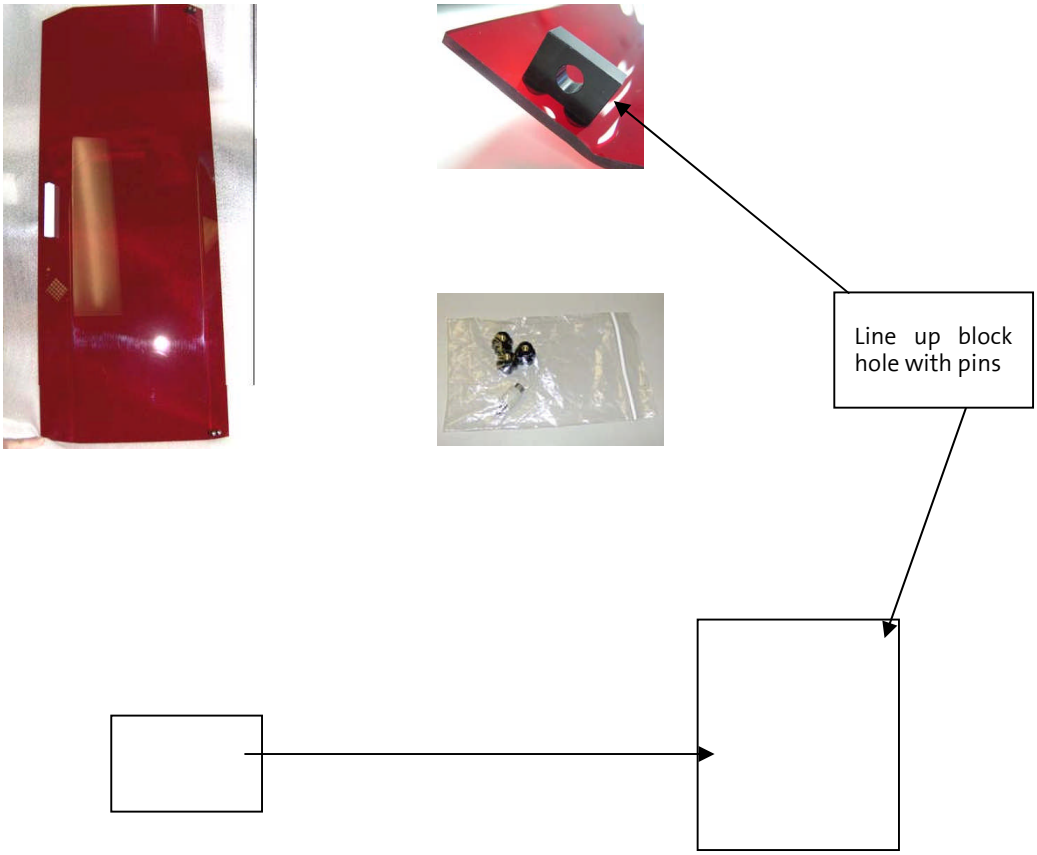

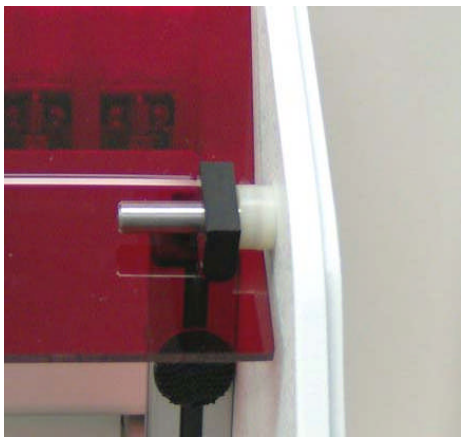

HUMAN
Gesellschaft für Biochemica und Diagnostica mbH
| Max-Planck-Ring 21 · 65205 Wiesbaden · Germany
| Tel.: +49 61 22/99 88-0 · Fax: +49 61 22/99 88-100
| e-Mail: human@human.de · www.human.de